



Certificate of Analysis


Sample: Chelan Gold
Date Tested: 2/8/2015
Test Result UID: ANL20150206C062595
WSLCB Tracking: 6033 4487 7000 0152

<http://anl360.com/349946>


Photographs



25x

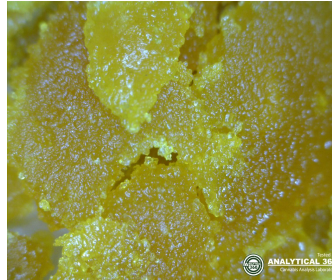


50x

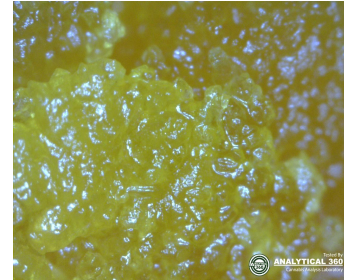

230x

HPLC Chromatogram

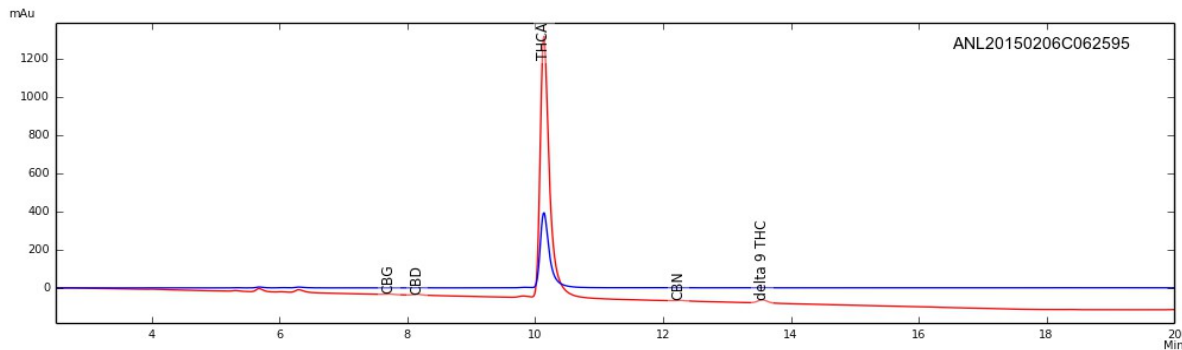


Cannabinoid Potency

81.71% Delta-9 THC Acid	< 0.01% CBD-Acid
1.55% Delta-9 THC	0.43% CBD
< 0.01% CBN	0.43% CBD-Total
83.26% THC-Total	< 0.01% CBC
0.22% CBG	2.20% Activated Total (Δ 9THC + CBN + CBD + CBC)
73.21% Active cannabinoids (THC-A x (0.877) + THC)	



Certificate of Analysis – Residual Solvent Analysis

Sample: Chelan Gold
Date Tested: 2/8/2015
Test Result UID: ANL20150206C062595
WSLCB Tracking: 6033 4487 7000 0152
GC Chromatogram

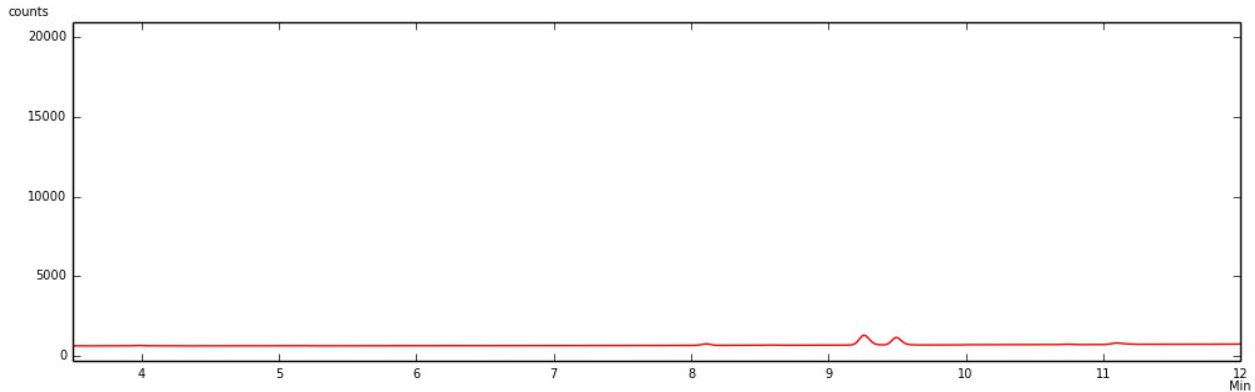

- <10 **PPM Propane**
- <10 **PPM Isobutane**
- <10 **PPM Butane**
- <10 **PPM Ethanol**
- <10 **PPM Acetone**
- <10 **PPM Isopentane**
- <10 **PPM Pentane**
- <10 **PPM Isopropanol**
- <10 **PPM Hexane**
- <10 **PPM Naphtha**
- <10 PPM SOLVENTS - TOTAL**

Daily Allowable Limits:

Propane:	500 ppm per day
Isobutane:	500 ppm per day
Butane:	500 ppm per day
Ethanol:	500 ppm per day
Acetone:	500 ppm per day
Isopentane:	500 ppm per day
Pentane:	500 ppm per day
Isopropanol:	500 ppm per day
Hexane:	290 ppm per day



Tested By

ANALYTICAL 360

Cannabis Analysis Laboratory

Certificate of Analysis

Sample: Chelan Gold
Date Tested: 2/8/2015
Test Result UID: ANL20150206C062595
WSLCB Tracking: 6033 4487 7000 0152

Foreign matter inspection: 0 % PASS

Microbial screen:

Total aerobic plate count	<25 CFUs/gram	PASS
Total yeast and mold count	<25 CFUs/gram	PASS
Bile-tolerant gram negative bacteria count	<25 CFUs/gram	PASS
Coliforms	<25 CFUs/gram	PASS
E. coli	ND	PASS
Salmonella spp.	ND	PASS

*Limits

ND= not detected

Foreign matter not more than 5.0 % of stems 3 mm or more in diameter; not more than 2.0 % of other foreign matter

Not more than 15 % moisture

Microbial

Not to exceed 100,000 Total aerobic plate count, 10,000 Total yeast and mold count, 1,000 bile-tolerant gram negative bacteria, 1,000 coliforms, and E coli and Salmonella not detected in one gram

Approved by: Dr. Lara M Taubner